

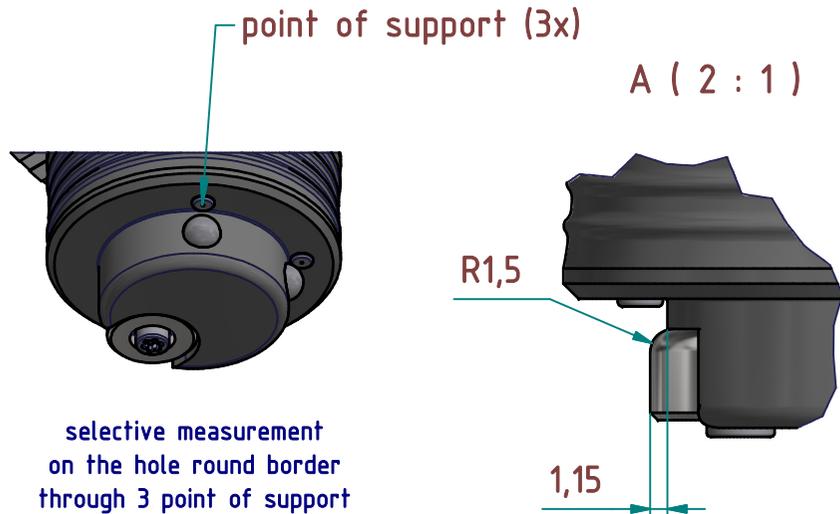


calibration with a adjusting ring 0641-31  
(included in delivery)

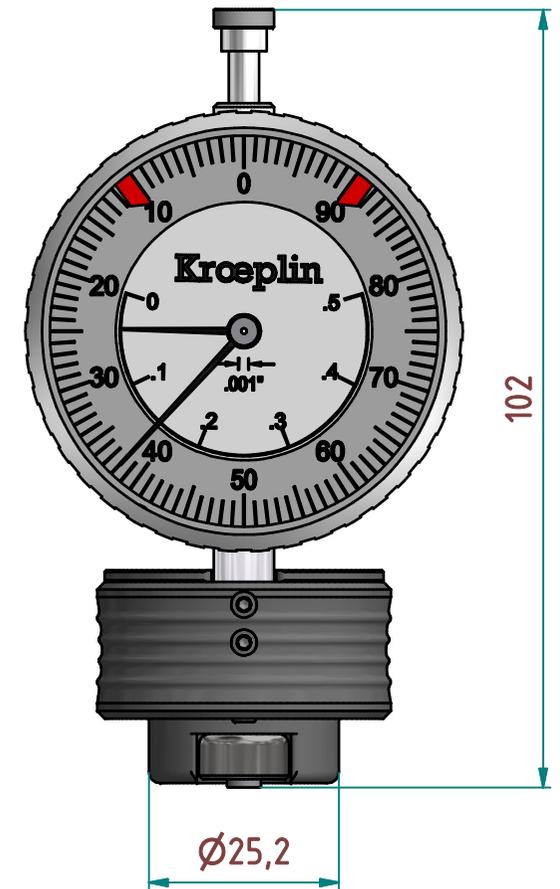

selective measurement  
on the hole round border  
through 3 point of support

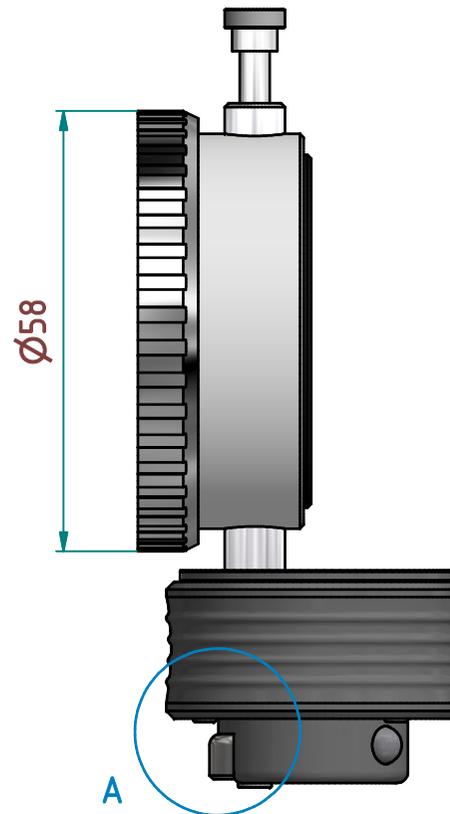

subject to technical alterations

**type:** aerosol  
**range:** .138 - .200 INCH  
**range of indication:** .122 - .400 INCH  
**digital step:** -  
**scale interval:** .001 INCH  
**measuring force:** 2,0 - 5,0 N  
**weight:** 300g

acceptable deviations  
VDI/VDE/DGQ 2618 Bl. 12.1/13.1)  
**max. permissible errors "G":** .001 INCH  
**repeatability "r":** .001 INCH  
**reference temperature:** 20° C  
**operation temperature:** 10° C - 30° C  
**storage temperature:** -10° C - 50° C

**scale:** 1 : 1  
**drawing-nr.:** A2130i-DB\_e  
**date of issue:** 14.07.15  
**name:** A.Wess  
**revision status:** 2123 / MHe  
**revision date:** 01.10.2015

4

3





2

1

A2130



calibration

measurement

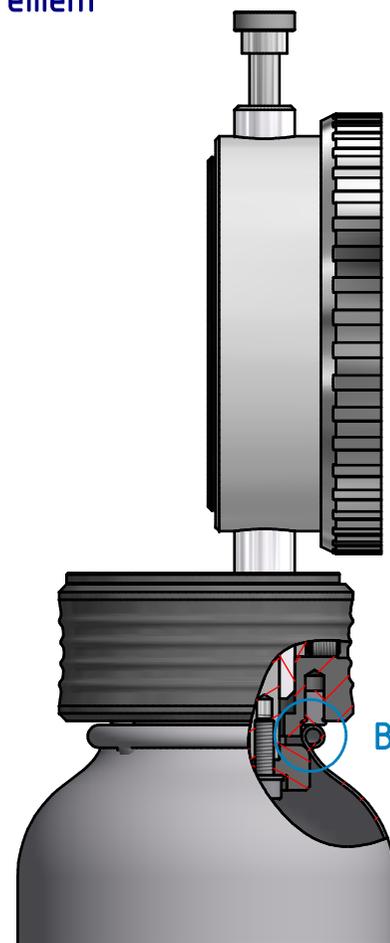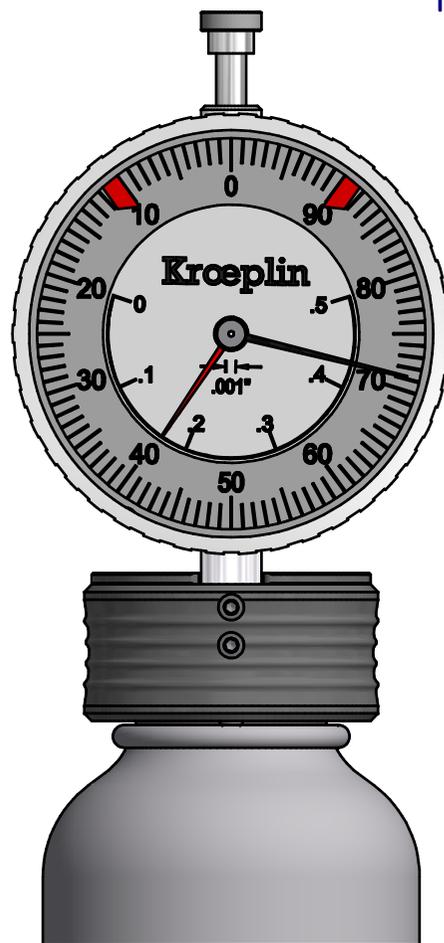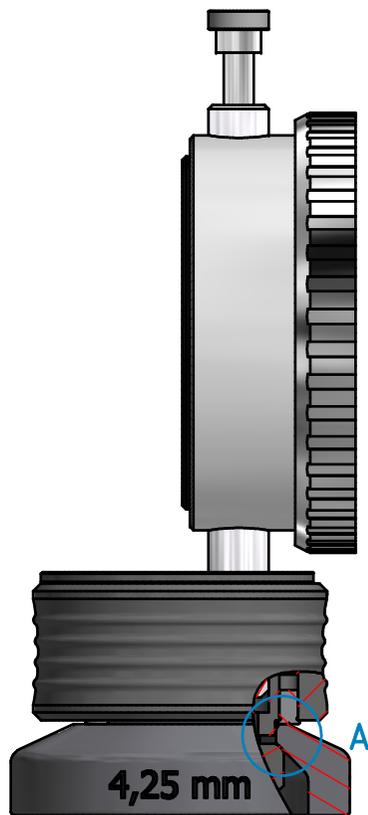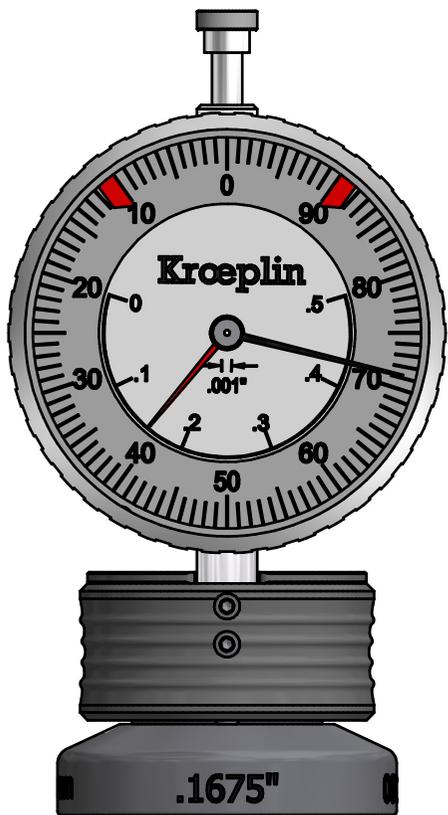

A (2 : 1)

B (2 : 1)

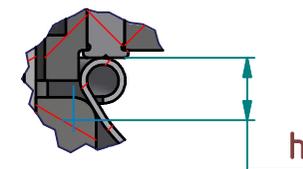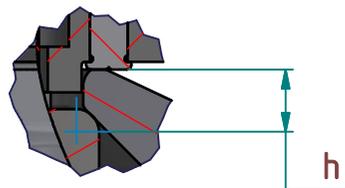

D

C

B

A