

# data sheet: AE1168i

measurement on  
20 mm aerosol can

Kroeplin GmbH  
Gartenstraße 50  
D-36381 Schlüchtern

Tel.: 06661 86 0  
Fax: 06661 86 39  
Mail: sales@kroeplin.com  
Web: www.kroeplin.com

**Kroeplin**  
Längenmesstechnik

157,55 [6.203]

Ø60 [2.362]

73 [2.874]



page 1

subject to technical alterations

type: aerosol  
range: .1575 - .3345 INCH  
range of indication:  
digital step: .0005 INCH  
scale interval:  
measuring force: 4-10 N  
weight: ca. 550 g

acceptable deviations  
VDI/VDE/DGQ 2618 Bl. 12.1/13.1)  
max. permissible  
errors "G": .002 INCH  
repeatability "r": .001 INCH  
reference temperature: 20° C  
operation temperature: 10° C - 30° C  
storage temperature: -10° C - 50° C

scale: 1:1  
drawing-nr.: IDW-AE1168i-DB\_e  
date of issue: 04.08.2016  
name: J.Röder  
revision status: 2310 (CT)  
revision date: 28.02.2024

4


3

2

1

## AE1161i – AE1169i chart of types

instrument, Order-No.	mouth-diameter: "Dm"	reference-diameter "DRef"	reference - height "HRef"	Order-No. jaws (Pos2)	Order-No. Holding-down clamp	a [mm]	Order-No. Calibration-part
AE1161 AE1161 i	14 mm	13,50 mm .5315 inch	5,00 mm .19685 inch	0840-14	0840-11	5	0761-32
AE1162 AE1162 i	15 mm	14,70 mm .5787 inch	7,00 mm .27559 inch	0840-10	0840-19	5	0761-40
AE1163 AE1163 i	16 mm	15,00 mm .5905 inch	5,00 mm .19685 inch	0840-17	0840-19	5	0761-38
AE1164 AE1164 i	16 mm	15,40 mm .6063 inch	5,00 mm .19685 inch	0840-16	0840-11	5	0761-34
AE1166 AE1166 i	19 mm	18,20 mm .7165 inch	5,00 mm .19685 inch	0840-18	0840-19	5	0761-39
AE1167 AE1167 i	20 mm	19,00 mm .76 inch	5,12 mm .20157 inch	0840-03	0840-04	14,6	0761-23
AE1168 AE1168 i	20 mm	19,40 mm .7638 inch	7,00 mm .27559 inch	0840-12	0840-04	14,6	0761-41
AE1169 AE1169 i	20 mm	19,85 mm .7795 inch	5,00 mm .19685 inch	0840-02	0840-04	14,6	0761-15

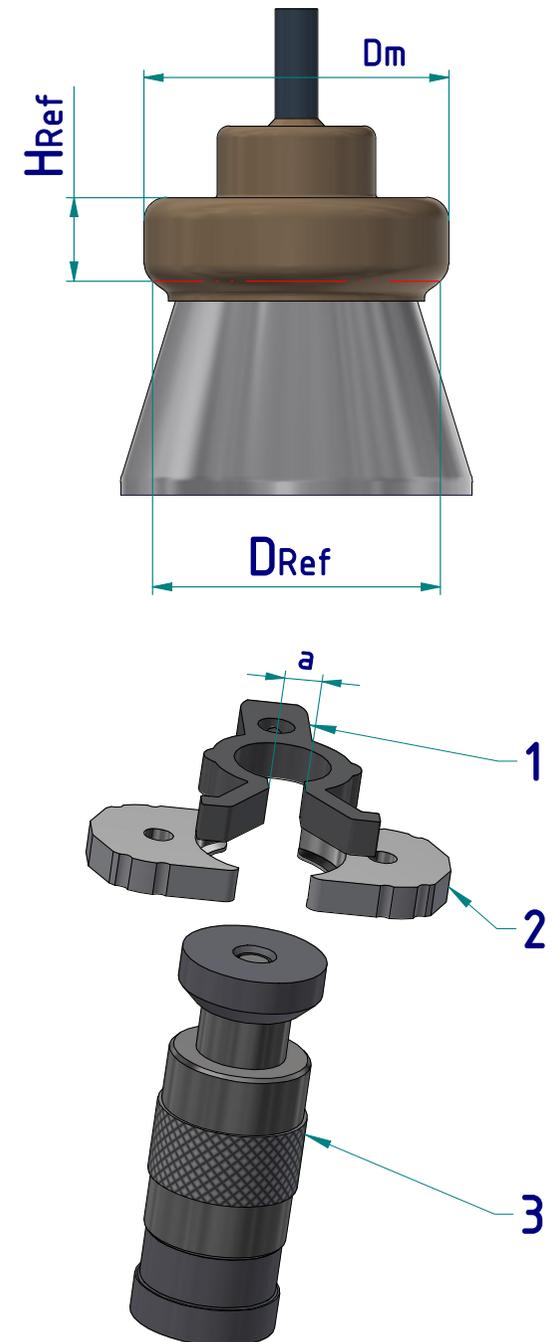

Please inquire further dimensions.

All instruments are supplied with corresponding jaws, holding-down clamp and calibration part in a wooden case.

A For conversion of a crimp test you need:

1 pc. holding-down clamp

2 pcs. jaws

1 pc. calibration part