

data sheet: AE2105

measurement of the Clinchhight CH
FEA 222 D


Kroepelin GmbH
Gartenstraße 50
D-36381 Schlüchtern

Tel.: 06661 86 0
Fax: 06661 86 39
Mail: sales@kroepelin.com
Web: www.kroepelin.com

Kroepelin
Längenmesstechnik

alternative calibration with
adjust ring
(not included in delivery)

order number: 0641-32

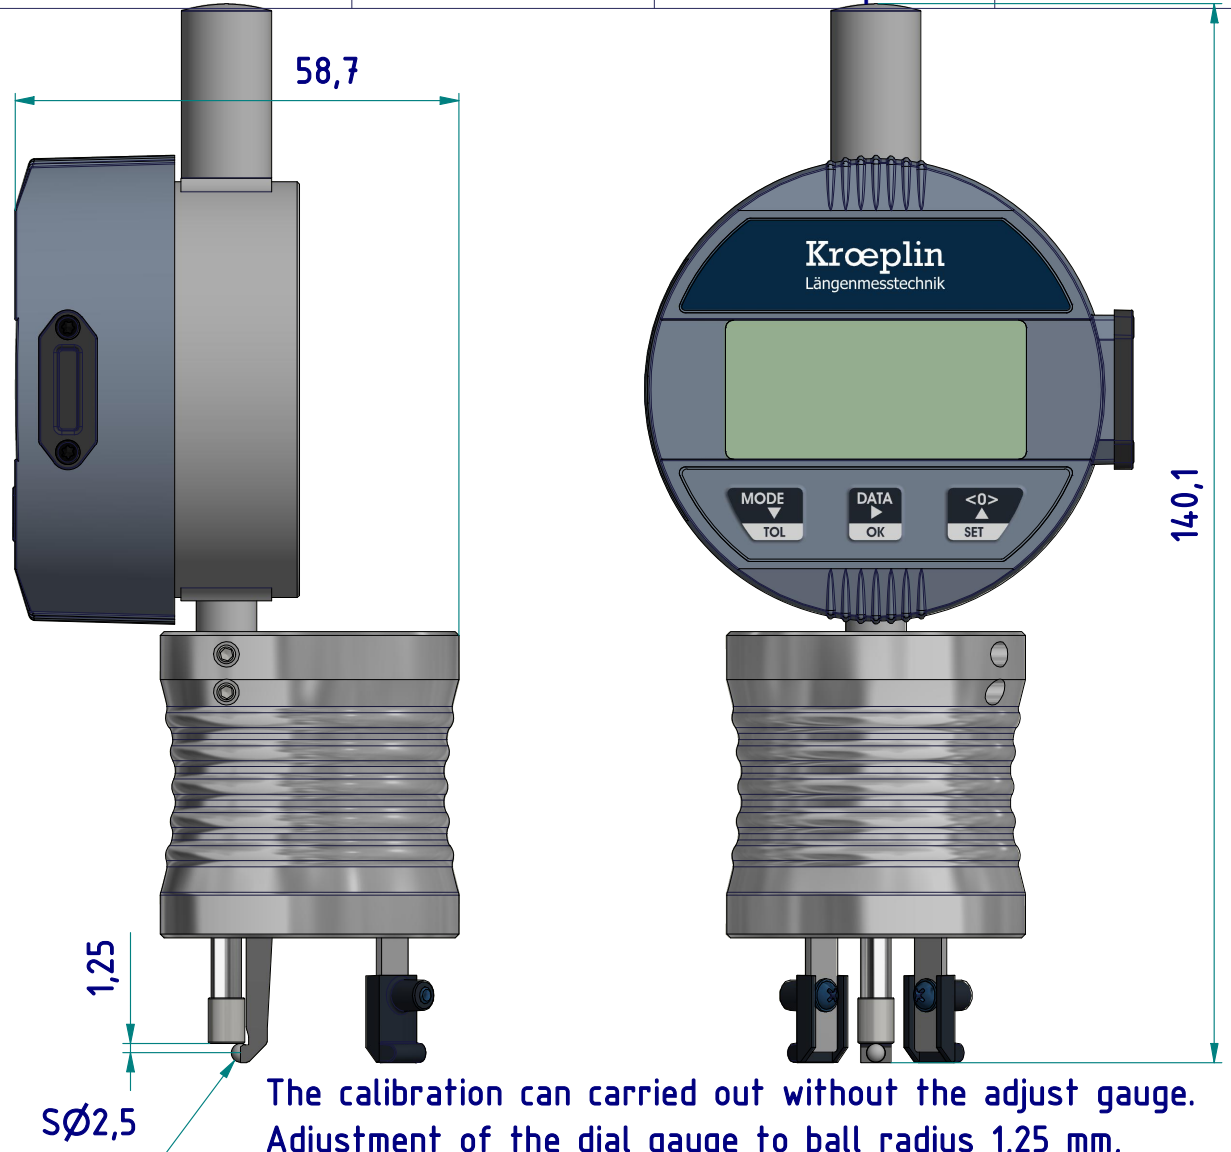

subject to technical alterations

The calibration can be carried out without the adjust gauge.
Adjustment of the dial gauge to ball radius 1,25 mm,

type: aerosol
range: 4,6 - 5,4 mm
range of indication: 1,25 - 10,3 mm
digital step: 0,01 mm
scale interval:
measuring force: 0,7 - 1,3 N
weight: ca. 280 g

acceptable deviations
VDI/VDE/DGQ 2618 Bl. 12.1/13.1)
max. permissible errors "G": 0,02 mm
repeatability "r": 0,02 mm
reference temperature: 20° C
operation temperature: 10° C - 30° C
storage temperature: -10° C - 50° C

scale: 1:1
drawing-nr.: IDW-AE2105-DB_e
date of issue: 25.11.2010
name: J.Heuser
revision status: 2310 (CT)
revision date: 13.03.2024

4

3

2

1

AE2105

calibration with
adjust gauge

measurement

D

C

B

A



A (2:1)

